

Quality is more than a word

ESPEC

Platinous J Series

Temperature & Humidity Chamber
Low/Ultra Low/High/Low Humidity/Clean Temperature (& Humidity) Chamber



3 YEAR WARRANTY

 **LOW GWP**
REFRIGERANT

ESPEC Platinous J Series - Your best choice to cover broad reliability test applications. It offers flexible configurations to meet the needs of today and tomorrow.

To minimize our chambers potential environmental impact

R-449A is the best alternative to R-404A

Low GWP Refrigerant



R-449A is available on request.
(PR/PL/PSL/PU/PG only)



*R-449A is available on request

Type 1



Type 2



Contents

● Models Configuration	p.3 to 4
● Features	p.5 to 7
● Special Models	p. 8
● Controller	p.9
● Network	p.10
● Flexibility at its best	p.11 to 14
● Specifications	p.15 to 22
● Installation Requirements	p.23
● Installation Simulation(AR)	p.24
● Fittings / Accessories	p.25
● Options	p.26 to 37
● Options Check Sheet	p.38 to 40
● Larger model	p.41
● For IoT/5G	p.42

Type 3



Type 4



Models Configuration

	Model	Temperature
Temperature & Humidity Chambers	Temperature & Humidity Chamber PR-1J / PR-2J / PR-3J / PR-4J	-20°C to +100°C (-20°C to +150°C (optional)) (-20°C to +180°C (optional)) On request Up to +200°C
	Low Temperature & Humidity Chamber PL-1J / PL-2J / PL-3J / PL-4J	-40°C to +100°C (-40°C to +150°C (optional)) (-40°C to +180°C (optional)) On request Up to +200°C
	Ultra Low Temperature & Humidity Chamber PSL-2J / PSL-4J	-70°C to +100°C (-70°C to +150°C (optional)) (-70°C to +180°C (optional))* On request Up to +200°C
	High Temperature & Humidity Chamber PHP-2J / PHP-3J / PHP-4J	ambient temperature +10°C to +100°C
	Low Humidity Type Temperature & Humidity Chamber PDR-3J / PDR-4J	-20°C to +100°C
	Low Humidity Type Low Temperature & Humidity Chamber PDL-3J / PDL-4J	-40°C to +100°C
	Clean Temperature & Humidity Chamber PCR-3J [Cleanliness: Class5 (HEPA Filter)]	-20°C to +100°C
	Temperature Chambers	Low Temperature Chamber PU-1J / PU-2J / PU-3J / PU-4J
Ultra Low Temperature Chamber PG-2J / PG-4J		-70°C to +100°C (-70°C to +150°C (optional)) (-70°C to +180°C (optional))* On request Up to +200°C

* Applicable only to Type 2

Humidity		Inside capacity
<p>20%rh to 98%rh</p> <ul style="list-style-type: none"> • With no specimen and under ambient temperature at +23°C. • Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler. 		<p>Type 1: 120 L Type 2: 225 L Type 3: 408 L Type 4: 800 L</p> <p>On request 816 L 1000 L</p>
<p>40%rh to 98%rh</p> <ul style="list-style-type: none"> • With no specimen. 		<p>Type 2: 306 L Type 4: 800 L</p> <p>Type 2: 219 L Type 3: 398 L Type 4: 784 L</p>
<p>5%rh to 98%rh*</p> <ul style="list-style-type: none"> • With no specimen and under ambient temperature at +23°C. • Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler. 		<p>Type 3: 408 L Type 4: 800 L</p>
<p>30%rh to 90%rh</p> <ul style="list-style-type: none"> • With no specimen and under ambient temperature at +23°C. • Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler. 		<p>Type 3: 312 L</p>
		<p>Type 1: 120 L Type 3: 408 L Type 2: 225 L Type 4: 800 L</p>
		<p>Type 2: 306 L Type 4: 800 L</p>


*) Low Humidity Region Operation Precautions

- Operation in the low humidity region is not possible from a high temperature above +60°C. Perform transition from temperatures below +60°C.
- Gradient programs cannot be used in the low humidity region. • Programs that require humidifier switching cannot be used. • Programs that transit from outside the low humidity region to the low humidity region cannot be used. However, the transition from the low humidity region to another region is allowed.


Features

Energy-saving Technologies


● New Refrigeration Circuit

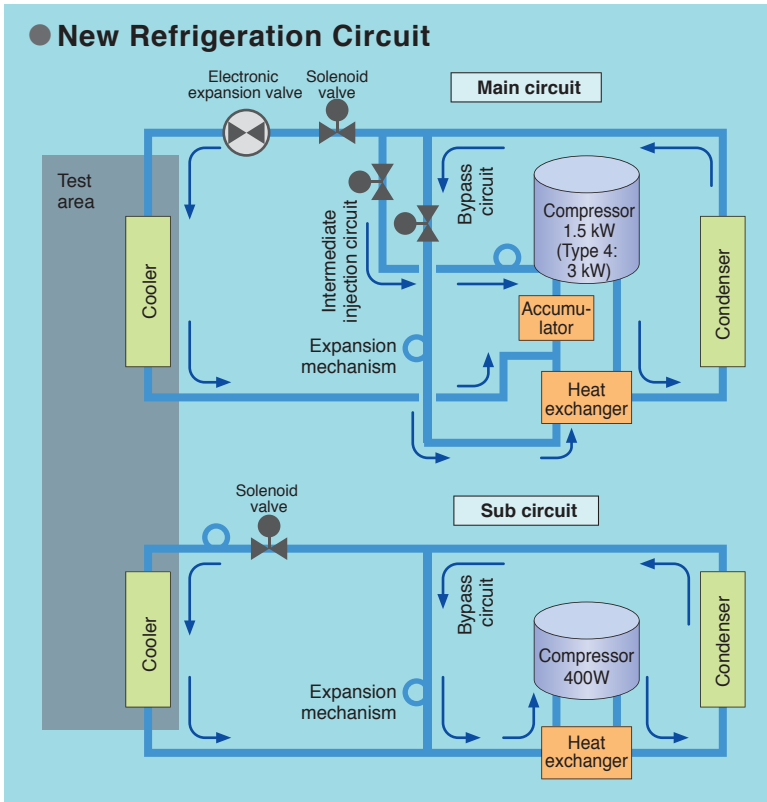

● Power Consumption Comparison (example)

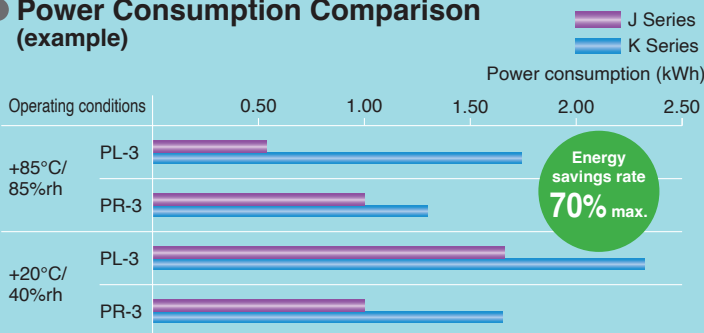

● Energy-saving DC Inverter Refrigeration

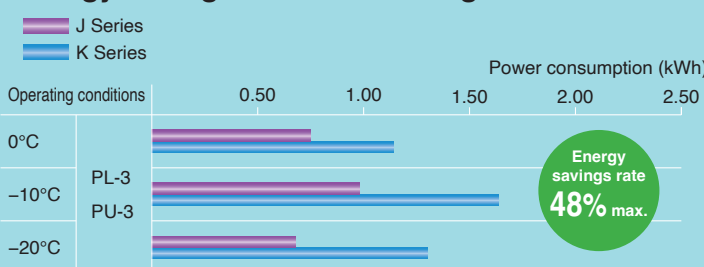

● Smart R&D System (Japanese patent no. 5514787)

Smart R&D System (Smart Refrigerator & Dehumidifier System) is the ESPEC patent, which can control both cooling and heating capacity at minimum limits. It provides highly accurate temperature / humidity environment with low energy consumption. The system consists of PID controlled refrigerator, and N instrumentation, which delivers high speed processing.

● A Sub Refrigeration Circuit PL-2/3/4, PU-2/3/4, PSL, PG, PDL, PCR

The chambers equip another energy-saving technology, a sub refrigeration circuit controlled by "Smart R&D System" with a 400W compressor. When the chamber operation is stable at constant ranges above 50°C / 40%rh, it switches to sub refrigeration to run at minimum energy. For example, the PL-3J power consumption can be cut by 70% max. (compared to previous K series)

The Japan Machinery Federation The Energy-Efficient Machinery Award



優秀省エネルギー機器

● DC Inverter Refrigeration (Option, 200V only) PL-2/3/4, PU-2/3/4

If the chamber is often used in low temperature ranges, the DC inverter refrigeration is a better option for excellent energy saving performance in low temperature ranges.

Features

● Viewing Window as Standard

Equipped with viewing window as standard, and chamber lamp (LED lamps) provide greater visibility.



Viewing window

● A Variety of Door Types

Several types of chamber doors are available for selection: a standard type with viewing window, a door without a viewing window, and a wide-view door that allows you to check the inside of the whole test area.

Furthermore, you can customize the door according to your application by, for example, adding hand-in ports to the door or installing an inner glass door to the chamber door. (Page 11-12, 27-28)



Wide-view door (option)



Door without viewing window (option)

● Humidifier Delay Function

Humidifier operation starts after the temperature is attained in order to reduce dew condensation on specimens.

● Automatic Humidifier Water Replacement

Humidifier stagnant water contains impurities and is a cause of trouble, so the chamber now features a function that automatically replaces the water at the period set from the controller screen.

● A Choice of Several Water Supply Systems

Several options to supply water to the chamber are offered, including direct tap water connection, pure water, additional tanks, etc.



Water tank



Additional water supply tank (option)

Features



Wick inside chamber



Condenser filter



Door handle lock




Power key switch (option)



Electro-chemical Migration Evaluation System connection (example)

● Facile Wick Replacement PR, PL, PSL, PHP (Japanese patent no. 5571634)

The difficulty in replacing the wet-bulb wick has been improved by changing the shape of the wick's plug part to allow smooth replacement work.



FW-5



● Easy Filter Cleaning

The condenser filter can be easily attached and removed from the chamber to make cleaning even easier.

● Door & Power Supply Locks

Door lock prevents accidental interruption during testing.

The double-lock door handle is designed to close the door more easily and safely. As an option, a power key switch can also be equipped to control the chamber's power.

● Combination with ESPEC Evaluation Systems

Even more accurate Electro-chemical migration evaluations can be performed by connecting a Platinum J Series to our AMI System (sold separately).


If the chamber equips with an optional cable port on the right side, the cables can be accessed from both right and left sides of AMI system.

Special Models

Energy saving and long term applications such as 85°C/85%rh

PHP

Heat pipes are used for the cooling system, which means that the refrigeration system does not use electrical power. Furthermore, it enables high temp./humid. testing such as 95°C / 95%rh as heat pipes barely dehumidify in cooling.

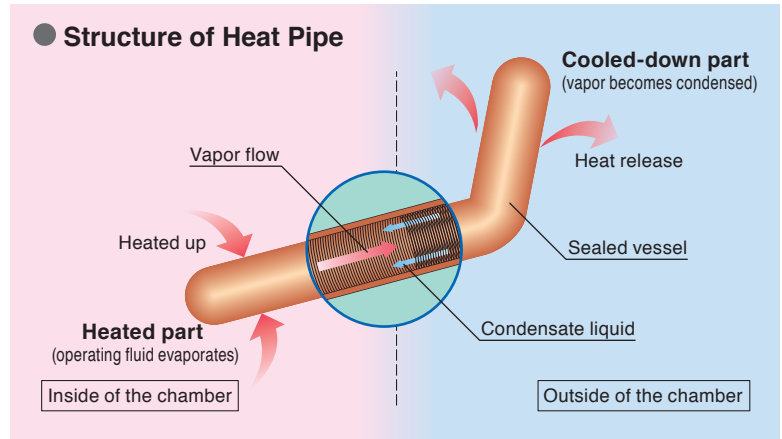

ISO Class 5 Cleanliness

PCR

PCR employs a HEPA filter to realize ISO Class 5 cleanliness in stable temp. & humid. control.



Clean Temperature & Humidity Chamber (PCR)

Superior Low-humidity Control Performance

PDR·PDL

With the independently-developed rotary regenerative dehumidifier method, low-humidity control is realized such as 60°C / 5%rh. (Control range chart is on page 4 & 19.)



As an option, further low temp. & humid. range (up to 5°C / 5%rh) can be controlled (page 32.)



Low Humidity & Low Temperature Chamber (PDL)


Controller

Easy-to-use, easy-to-read touch panel

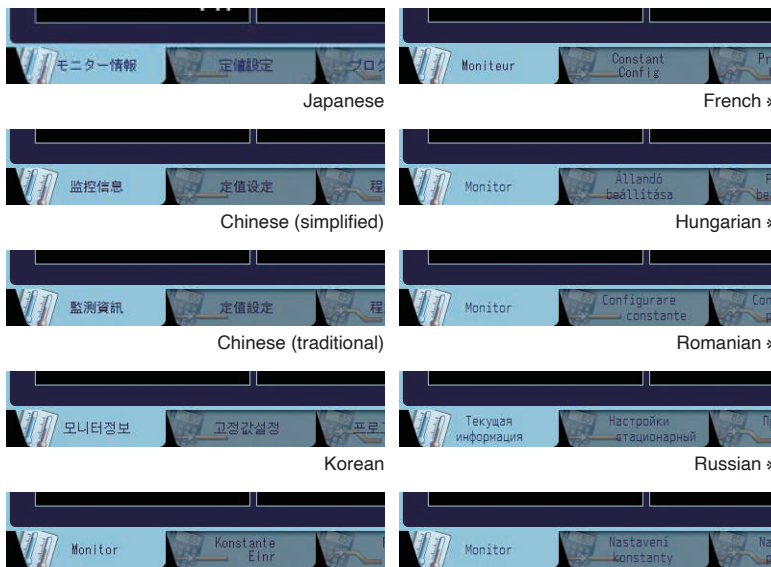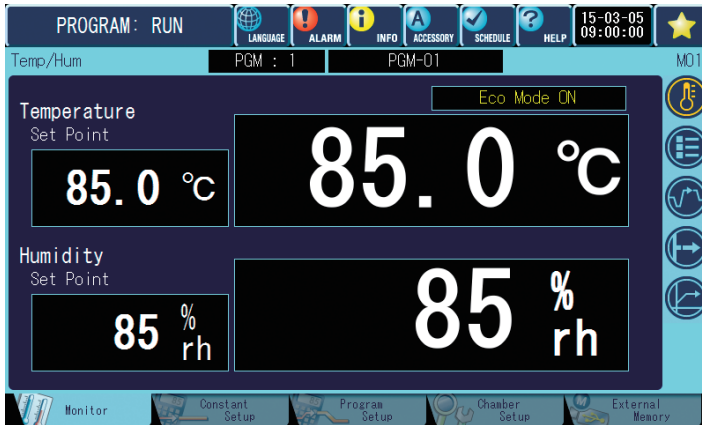

* Available on request

● Program Copying and Computer Editing

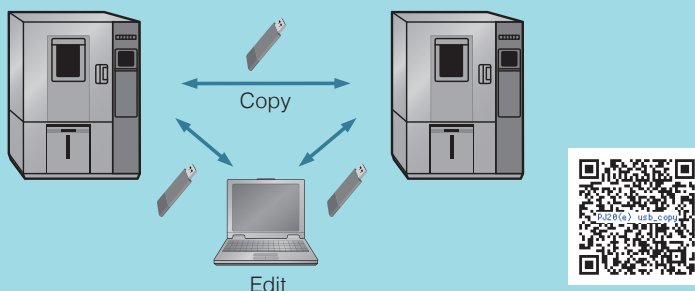

● Tabbed Interface

High resolution 7 inch LCD. Tabs are displayed at the bottom of the screen to help access to other screens.

A touch navigation bar is also displayed along the right of the screen to access principal pages anytime.

● Information Function

The INFO icon will blink when chamber information requiring attention.

- Inspection Period Notifications

It is possible to randomly preset the period and details of inspections for humidifier plates and condenser filters.

- Status Notifications

Defrosting, auto-humidifying water replacement, and so on.

● Test Data Records & Exports

Temp. & humid. settings and measured values are recorded on controller's internal memory. The data and its graph can be exported to USB flash drives.

* Interval can be changed.

● Program Patterns Copying

Program patterns can be copied between chambers with the use of USB flash drives without using a computer.

● PATTERN MANAGER Lite

It is a PC software that makes the most of the USB port.

Outside of any networks, the test data exported via USB flash drive can be checked and graphed on PC. You can also change the chamber's set values and import the edited data to chambers.

The program patterns in accordance with test standards are available on our web site, "Test Navi"

Enable to Monitor & Operate from Web Browser

Remote Monitoring and Control (Ethernet Connection)

The chambers are equipped with unique web applications that enable chamber status to be confirmed and operated from a web browser screen (PC or tablet terminal). It is also possible to start operations with a PC or other device from a remote location.

Editing Test Profiles with a Browser

It is possible to edit the program patterns registered in the testing chamber with a web browser.


Displaying Data in Graphs

Settings and measurement values saved in the testing chamber can be displayed as graphs on a web browser.

E-mail Notifications

Details on alarms that have been triggered will be sent to pre-registered e-mail addresses. It is also possible to transmit e-mails when testing has finished.

* An Intranet environment is required to transmit e-mails.

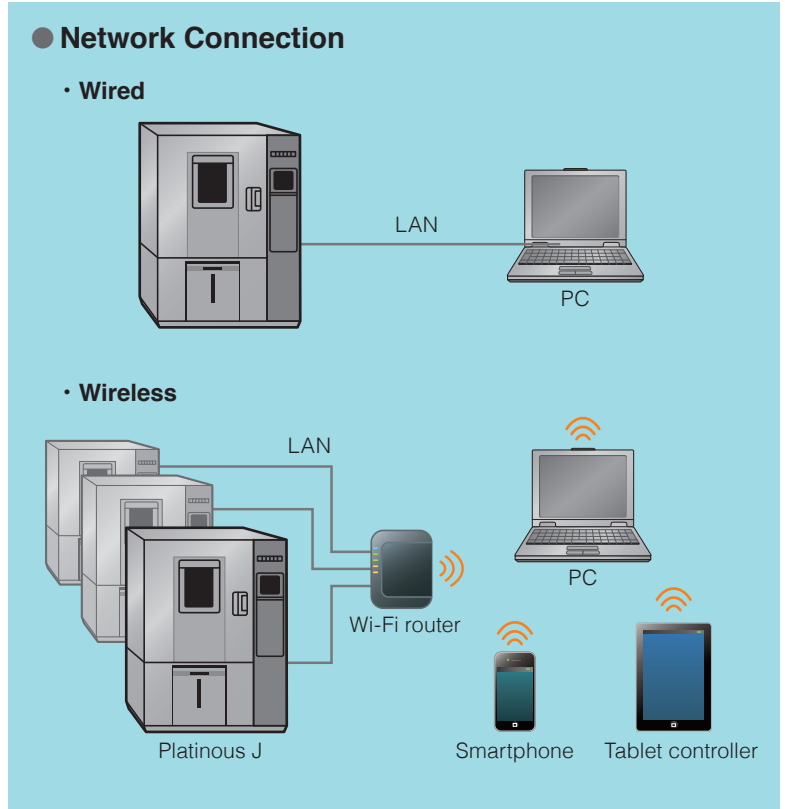


Login Privileges of Web Browser

Screen / Privileges	Chamber monitor	Constant/ Program setup	Run/Stop	Configuration
Administrator	✓	✓	✓	✓
Operator	✓	✓	✓	
User	✓			

ESPEC OnlineCore (Sold separately)

Central control system recommended for multiple environmental test chambers installations

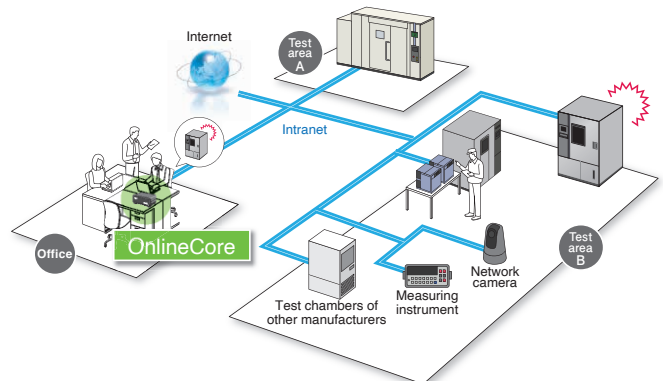

Options – Flexibility at its best –

For Better Operability



In addition to standard specifications, a wide selection of options is available to enhance functions and meet specific testing needs. Test equipment performance can also be enhanced to make it more accurate, multi-functional, or capable of a greater load as designed.

1 Ceiling cable port →P.30

2 Left-side cable port (standard) →P.30

3 EZ connect cable port plug for power supply
 This mounting/dismounting terminal can be additionally installed on the left side cable port. It simplifies to connect the wiring for voltage or measurement equipment to the specimens located inside the chamber.
 →P.31



4 Wide-view door
 An all-glass wide-view door provides an unrestricted view of every bit of space inside the chamber. Temperature differential with the outside of the chamber can be controlled to suppress the formation of condensation on the glass surface.
 →P.27

Wide-view door with hand-in ports (Japanese patent No.4137894)


This option features hand-in ports on a standard door, to manipulate the specimen even during testing.
 →P.27

Options – Flexibility at its best –

5 Specimen basket

The basket can be placed on a shelf to hold small specimens.

→P.29

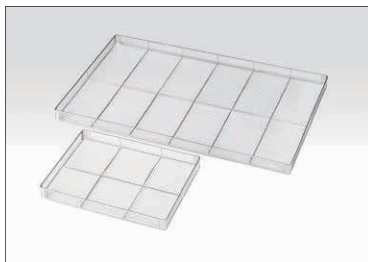

6 Shelf

Shelve(s) can be placed in the sides of the test area to hold specimens.

→P.29



7 Paperless recorder

Records internal temperature and other temperature (and humidity).

→P.34

8 Applying DC power supply

Used to apply voltage to specimens for bias testing. The output mode and interlock conditions can be set for the DC power supply in each step of the temperature and humidity program.

→P.33

9 Right-side cable port

A cable port in the right side of the chamber.

→P.30

* The standard cable port is located in the left side.



10 Specimen temperature control

A temperature sensor, which will be connected directly to specimen. It enhances the accuracy of temperature tests.

→P.33

11 Power meter

Shows the chamber integral power consumption.

→P.34

12 Folding table

A folding table is provided on the right side of the chamber. It can be used to hold measuring instrument, a computer, or other devices connected to the chamber.

→P.34



13 100 V power sockets

Two 100 V power sockets can be used to supply power for specimen and/or measuring instruments. One circuit protector is also equipped.

→P.26

Wide-view door up to +150°C

Expand temperature range up to +150°C. Hand-in ports and roller blind options are available.



Options – Flexibility at its best –

Safety of Operators and Protection of Specimens



Safety functions depend on the specimen characteristics. A wide variety of options is available to protect the chamber in the case of specimens that generate corrosive substances, to protect the specimens and the chamber during testing, and to ensure the safety of the operator(s).

1 Door handle (standard)

Large handle provides a better grip. A double lock provides secure opening and closing.



2 Door lock (standard)

Prevents door opening during testing.

3 Status indicator light

Indicator tower provides a view of the chamber status from a remote location. Light color, light status (on, blinking), buzzer on/off can be configured as required.

→P.35



Options – Flexibility at its best –

④ Specimen power supply control terminal (standard)

If the chamber sends an error alert, the equipment's power supply connected through this terminal is shut down immediately.



⑤ Overheat protector (standard) Additional overheat protector

Specimen protection is enhanced by an additional overheat protector.



⑥ Overcool protector

Operation will stop to protect specimens whenever temperature in the test area drops below a setting temperature for some reason.

⑦ Emergency stop pushbutton

Switch for manual emergency stop of the chamber. Also available with a guard or cover to prevent unintended operation.



⑧ Alarm output terminal

This contact signal terminal is for sending error alerts to a remote location during safety actions.

→P.35

⑨ Power indicator

Indicates the breaker on/off status from the front of the chamber.



⑩ Power key switch

Installation of the power supply key enables management of the chamber use.








⑪ Dehumidifier electrical compartment door switch (standard)

A breaker turns off to protect against electric shock if a door open state is detected.



PR

-20°C to +100°C (+150°C / +180°C) • 20%rh to 98%rh TEMPERATURE & HUMIDITY CHAMBER

Model	PR-1J	PR-2J	PR-3J	PR-4J	
System	Balanced Temperature and Humidity Control system (BTHC system)				
Performance ^{*1}	Temp. & humidity range	-20°C to +100°C/20%rh to 98%rh ^{*2} Refer to diagram of temperature & humidity controllable range on this page.			
	Temp. & humidity fluctuation	±0.3°C/±2.5%rh			
	Temperature variation in space	1.5°C			
	Temperature rate of change	Heat up rate: 3.0°C/min. Pull down rate: 2.0°C/min.		Heat up rate: 3.0°C/min. Pull down rate: 1.0°C/min.	
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -20°C 40 min.			
	Allowable heat load ^{*3}	800 W	1100 W	1250 W	
Allowable ambient conditions	0°C to +40°C/up to 75%rh				
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish			
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish			
	Heater	Nichrome strip wire heater			
	Humidifier	18-12-2.5 Cr-Ni-Mo stainless steel sheathed heater (surface evaporating system)			
	Cooler (dehumidifier)	Plate fin cooler			
	Air circulator	Cross flow fan		Sirocco fan	
	System	Mechanical single-stage refrigeration system			
	Refrigerant	R-404A [R-449A is available on request]			
Capacity	120 L	225 L	408 L	800 L	
Chamber total load resistance	100 kg				
Dimensions ^{*4}	Inside dimensions (W x H x D mm)	500 x 600 x 400	500 x 750 x 600	600 x 850 x 800	1000 x 1000 x 800
	Outside dimensions (W x H x D mm)	910 x 1440 x 873	910 x 1590 x 1073	1010 x 1690 x 1273	1410 x 1840 (1970) x 1273
Weight	260 kg	305 kg	365 kg	480 kg	
Augmented Reality Learn more  page 24					
	▲Exterior view	▲Exterior view	▲Exterior view	▲Exterior view	


*1 The performance values are based on IEC60068-3-5:2001 and IEC60068-3-6:2001;

Performance figures are given for a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C

*3 When temperature in chamber is +20°C

*4 Excluding protrusions. Dimension indicated in () includes protrusion.

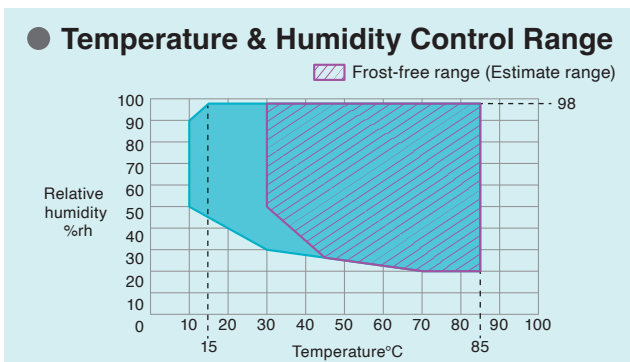

* With no specimen and under ambient temperature at +23°C.

* Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler.

Low GWP Refrigerant








R-449A is available on request.
(PR/PL/PSL/PU/PG only)

PL

-40°C to +100°C (+150°C / +180°C) • 20%rh to 98%rh

LOW TEMPERATURE & HUMIDITY CHAMBER

Model	PL-1J	PL-2J	PL-3J	PL-4J	
System	Balanced Temperature and Humidity Control system (BTHC system)				
Performance*1	Temp. & humidity range*2	-40°C to +100°C/20%rh to 98%rh Refer to diagram of temperature & humidity controllable range on this page.			
	Temp. & humidity fluctuation	±0.3°C/±2.5%rh			
	Temperature variation in space	1.5°C			
	Temperature rate of change	Heat up rate: 3.0°C/min. Pull down rate: 2.0°C/min.			
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -40°C 45 min.			
	Allowable heat load*3	850 W	1400 W	1500 W	2850 W
Allowable ambient conditions	0°C to +40°C/up to 75%rh				
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish			
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish			
	Heater	Nichrome strip wire heater			
	Humidifier	18-12-2.5 Cr-Ni-Mo stainless steel sheathed heater (surface evaporating system)			
	Cooler (dehumidifier)	Plate fin cooler	Plate fin cooler, stainless steel tube cooler		
	Air circulator	Cross flow fan		Sirocco fan	
	System	Mechanical type single-stage compression cooling			
	Refrigerant	Low GWP Refrigerant R-404A (R-449A is available on request)			
Capacity	120 L	225 L	408 L	800 L	
Chamber total load resistance	100 kg				
Dimensions*4	Inside dimensions (W x H x D mm)	500 x 600 x 400	500 x 750 x 600	600 x 850 x 800	1000 x 1000 x 800
	Outside dimensions (W x H x D mm)	910 x 1440 x 873	910 x 1590 x 1073	1010 x 1690 x 1273	1410 x 1840 (1970) x 1273
Weight	270 kg	340 kg	420 kg	610 kg	
Augmented Reality Learn more  page 24	 ▲Exterior view	 ▲Exterior view	 ▲Exterior view	 ▲Exterior view	

*1 The performance values are based on IEC60068-3-5:2001 and IEC60068-3-6:2001;


Performance figures are given for a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C

*3 When temperature in chamber is +20°C

*4 Excluding protrusions. Dimension indicated in () includes protrusion.

● Temperature & Humidity Control Range

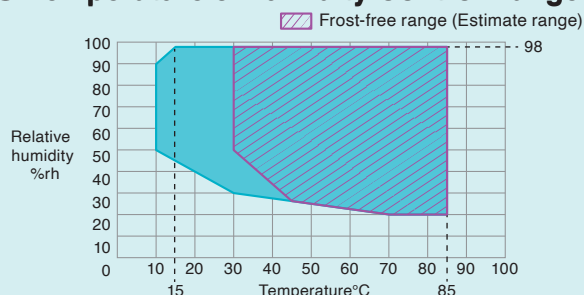




* With no specimen and under ambient temperature at +23°C.

* Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler.

Low GWP Refrigerant



R-449A is available on request.
(PR/PL/PSL/PU/PG only)

Model		PSL-2J	PSL-4J
System		Balanced Temperature and Humidity Control system (BTHC system)	
Performance ^{*1}	Temp. & humidity range ^{*2}	-70°C to +100°C/20%rh to 98%rh Refer to diagram of temperature & humidity controllable range on this page.	
	Temp. & humidity fluctuation	±0.3°C/±2.5%rh	
	Temperature variation in space	1.5°C	
	Temperature rate of change	Heat up rate: 5.0°C/min. Pull down rate: 2.0°C/min.	Heat up rate: 5.0°C/min. Pull down rate: 1.0°C/min.
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -70°C 65 min.	
	Allowable heat load ^{*3}	700 W	2200 W
Allowable ambient conditions		0°C to +40°C/up to 75%rh	
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish	
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish	
	Heater	Nichrome strip wire heater	
	Humidifier	18-12-2.5 Cr-Ni-Mo stainless steel sheathed heater (surface evaporating system)	
	Cooler (dehumidifier)	Plate fin cooler (Doubles as dehumidifier), stainless steel tube cooler	
	Air circulator	Cross flow fan	Sirocco fan
	System	Mechanical cascade refrigerator system	
	Refrigerant	R-404A (R-449A is available on request), R-508A	
Capacity		306 L	800 L
Chamber total load resistance		100 kg	
Dimensions ^{*4}	Inside dimensions (W x H x D mm)	600 x 850 x 600	1000 x 1000 x 800
	Outside dimensions (W x H x D mm)	1010 x 1690 x 1273	1410 x 1853 (1983) x 1593
Weight		470 kg	705 kg
Augmented Reality Learn more  page 24		 ▲Exterior view	 ▲Exterior view

*1 The performance values are based on IEC60068-3-5:2001 and IEC60068-3-6:2001;


Performance figures are given for a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C

*3 When temperature in chamber is +20°C

*4 Excluding protrusions. Dimension indicated in () includes protrusion.

● Temperature & Humidity Control Range

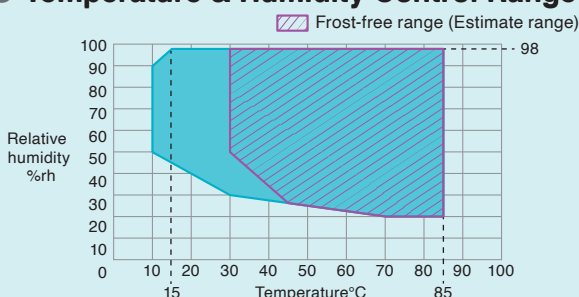





* With no specimen and under ambient temperature at +23°C.

* Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler.

Low GWP Refrigerant



R-449A is available on request.
(PR/PL/PSL/PU/PG only)

Model	PHP-2J	PHP-3J	PHP-4J	
System	Balanced Temperature and Humidity Control system (BTHC system)			
Performance*1	Temp. & humidity range	Ambient temperature +10°C to +100°C/40%rh to 98%rh Refer to diagram of temperature & humidity controllable range on this page.		
	Temp. & humidity fluctuation	±0.3°C/±2.5%rh		
	Temperature variation in space	1.5°C		
	Allowable heat load*3	300 W	600 W	
Allowable ambient conditions	0°C to +40°C/up to 75%rh			
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish		
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish		
	Heater	Nichrome strip wire heater		
	Humidifier	18-12-2.5 Cr-Ni-Mo stainless steel sheathed heater (surface evaporating system)		
	Cooler (dehumidifier)	Plate fin cooler (heat pipe system)		
	Air circulator	Cross flow fan	Sirocco fan	
Capacity	219 L	398 L	784 L	
Chamber total load resistance	100 kg			
Dimensions*4	Inside dimensions (W x H x D mm)	500 x 730 x 600	600 x 830 x 800	1000 x 980 x 800
	Outside dimensions (W x H x D mm)	910 x 1590 x 1073	1010 x 1690 x 1273	1410 x 1840 (1970) x 1273
Weight	275 kg	335 kg	490 kg	
Augmented Reality Learn more  page 24	 ▲Exterior view	 ▲Exterior view	 ▲Exterior view	

*1 The performance values are based on IEC60068-3-5:2001 and IEC60068-3-6:2001;


Performance figures are given for a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C

*3 When temperature in chamber is +20°C

*4 Excluding protrusions. Dimension indicated in () includes protrusion.

● Temperature & Humidity Control Range

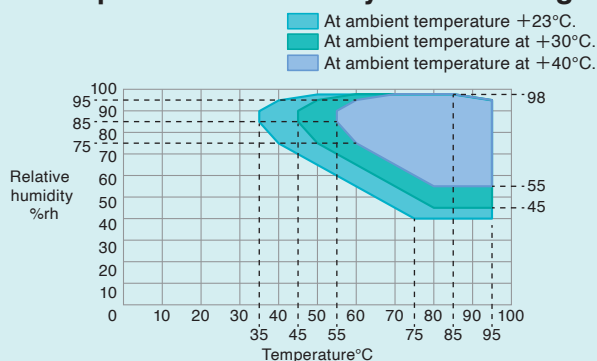






* With no specimen.

PDR·PDL

5%rh to 98%rh · -20°C to +100°C / -40°C to +100°C

LOW HUMIDITY TYPE (LOW) TEMPERATURE & HUMIDITY CHAMBER

Model	PDR-3J	PDR-4J	PDL-3J	PDL-4J	
System	Balanced Temperature and Humidity Control system (BTHC system)				
Performance ^{*1}	Temp. & humidity range ^{*2}	-20°C to +100°C/5%rh to 98%rh Refer to diagram of temperature & humidity controllable range on this page.		-40°C to +100°C/5%rh to 98%rh Refer to diagram of temperature & humidity controllable range on this page.	
	Temp. & humidity fluctuation	± 0.3°C/± 2.5%rh			
	Temperature variation in space	1.5°C			
	Temperature rate of change	Heat up rate: 3.0°C/min. Pull down rate: 2.0°C/min.	Heat up rate: 3.0°C/min. Pull down rate: 1.0°C/min.	Heat up rate: 3.0°C/min. Pull down rate: 2.0°C/min.	
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -20°C 40 min.		Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -40°C 50 min.	
	Allowable heat load ^{*3}	1100 W	1250 W	1500 W	2850 W
Allowable ambient conditions	Standard temperature and humidity region running: 0°C to +40°C/up to 75%rh Low temperature and humidity region running: +5°C to +32°C Absolute humidity no greater than 23g/kg				
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish			
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish			
	Heater	Nichrome strip wire heater			
	Humidifier	18-12-2.5 Cr-Ni-Mo stainless steel sheathed heater (surface evaporating system)			
	Cooler	Plate fin cooler (Doubles as dehumidifier)	Plate fin cooler (Doubles as dehumidifier), stainless steel tube cooler		
	Air circulator	Sirocco fan			
	System	Mechanical type single-stage compression cooling			
	Refrigerant	R-404A			
	Dehumidifier	System	Rotary recovery (adsorption) dehumidification		
		Refrigerator system	Mechanical single-stage refrigeration system		
Compressor		Rotary compressor (R-404A), Reciprocating compressor (R134a)			
Expansion mechanism		Temperature regulated automatic expansion valve			
Capacity	408 L	800 L	408 L	800 L	
Chamber total load resistance	100 kg				
Dimensions ^{*4}	Inside dimensions (W x H x D mm)	600 x 850 x 800	1000 x 1000 x 800	600 x 850 x 800	1000 x 1000 x 800
	Outside dimensions (W x H x D mm)	1885 x 1690 (1820) x 1273	2285 x 1840(1970) x 1273	1885 x 1690 (1820) x 1273	2285 x 1840 (1970) x 1273
Weight ^{*5}	680 kg	800 kg	735 kg	930 kg	
Augmented Reality Learn more  page 24					
	▲Exterior view	▲Exterior view	▲Exterior view	▲Exterior view	


*1 The products displayed in AR are temperature and humidity types, which are equipped with a temperature & humidity controller and water tank.*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C

*3 When temperature in chamber is +20°C

*4 Excluding protrusions. Dimension indicated in () includes protrusion.

*5 Total weight (temperature & humidity chamber and dehumidifier)

● Temperature & Humidity Control Range

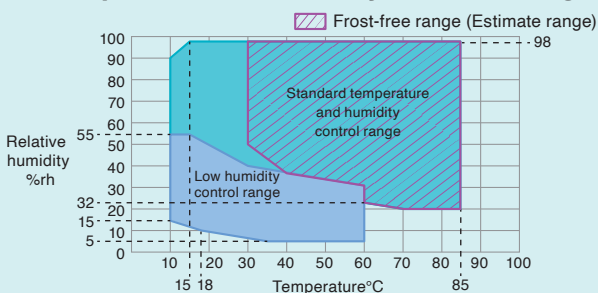



* With no specimen and under ambient temperature at +23°C.

* Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler.

Low Humidity Region Operation Precautions

- Operation in the low humidity region is not possible from a high temperature above +60°C. Perform transition from temperatures below +60°C.
- Gradient programs cannot be used in the low humidity region.
- Programs that require humidifier switching cannot be used.
- Programs that transition from outside the low humidity region to the low humidity region cannot be used. However, transitioning from the low humidity region to another region is allowed.

Model		PCR-3J
System		Balanced Temperature and Humidity Control system (BTHC system)
Performance ^{*1}	Temp. & humidity range ^{*2}	-20°C to +100°C/30%rh to 90%rh Refer to diagram of temperature & humidity controllable range on this page.
	Temp. & humidity fluctuation	±0.5°C/±2.5%rh
	Temperature variation in space	5.0°C
	Temperature rate of change	Heat up rate: 1.5°C/min. Pull down rate: 1.0°C/min.
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 55 min. Pull down time: from +20°C to -20°C 45 min.
	Cleanliness ^{*3}	Class5 (Particle diameter: 0.5 μm)
Allowable ambient conditions		+5°C to +35°C/up to 75%rh
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish
	Heater	Nichrome strip wire heater
	Humidifier	18-12-2.5 Cr-Ni-Mo stainless steel sheathed heater (surface evaporating system)
	Cooler (dehumidifier)	Plate fin cooler (Doubles as dehumidifier)
	Air circulator	Sirocco fan
	System	Mechanical type single-stage compression cooling
	Refrigerant	R-404A
Required exhaust equipment		Exhaust flow rate: 16m ³ / min. (50Hz);18m ³ /min. (60Hz); Chamber connection port: ø123mm
Capacity		312 L
Chamber total load resistance		100 kg
Dimensions ^{*4}	Inside dimensions (W x H x D mm)	600 x 650 x 800
	Outside dimensions (W x H x D mm)	1010 x 1880 x 1273
Weight		445 kg
Augmented Reality Learn more  page 24		 ▲Exterior view

*1 The performance values are based on IEC60068-3-5:2001 and IEC60068-3-6:2001; Performance figures are given for a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C


*3 When temperature is stable, the cleanliness is according to JIS B9920:2002 (equivalent to FED-STD-209D Class 100).

The Class 5 cleanliness cannot be maintained when the door is open.

Do not open the door when operating at temperatures below 0°C



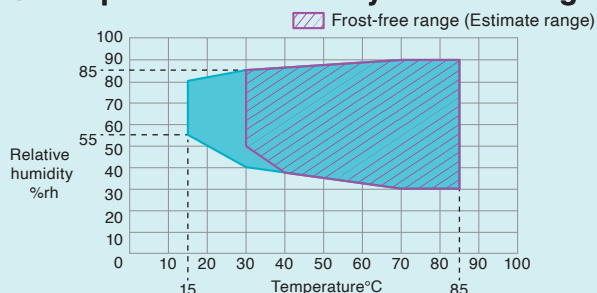


*4 Excluding protrusions.

● Temperature & Humidity Control Range



* With no specimen and under ambient temperature at +23°C.

* Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler.

Model	PU-1J	PU-2J	PU-3J	PU-4J	
System	Balanced Temperature Control system (BTC system)				
Performance ^{*1}	Temperature range ^{*2}	-40°C to +100°C			
	Temperature fluctuation	±0.3°C			
	Temperature variation in space	1.5°C			
	Temperature rate of change	Heat up rate: 3.0°C/min. Pull down rate: 2.0°C/min.			
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -40°C 45 min.			
	Allowable heat load ^{*3}	850 W	1400 W	1500 W	2850 W
Allowable ambient conditions	0°C to +40°C/up to 75%rh				
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish			
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish			
	Heater	Nichrome strip wire heater			
	Cooler (dehumidifier)	Plate fin cooler	Plate fin cooler, stainless steel tube cooler		
	Air circulator	Cross flow fan		Sirocco fan	
	System	Mechanical type single-stage compression cooling			
	Refrigerant	Low GWP Refrigerant R-404A (R-449A is available on request)			
Capacity	120 L	225 L	408 L	800 L	
Chamber total load resistance	100 kg				
Dimensions ^{*4}	Inside dimensions (W x H x D mm)	500 x 600 x 400	500 x 750 x 600	600 x 850 x 800	1000 x 1000 x 800
	Outside dimensions (W x H x D mm)	910 x 1440 x 873	910 x 1590 x 1073	1010 x 1690 x 1273	1410 x 1840 (1970) x 1273
Weight	260 kg	330 kg	410 kg	600 kg	
Augmented Reality Learn more  page 24	 ▲Exterior view	 ▲Exterior view	 ▲Exterior view	 ▲Exterior view	
As representation, the products displayed in AR are temperature and humidity types.					

*1 The performance values are based on IEC60068-3-5:2001 under the conditions of a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C




*3 When temperature in chamber is +20°C

*4 Excluding protrusions. Dimension indicated in () includes protrusion.

Low GWP Refrigerant



R-449A is available on request.
(PR/PL/PSL/PU/PG only)

Model		PG-2J	PG-4J
System		Balanced Temperature Control system (BTC system)	
Performance ^{*1}	Temperature range ^{*2}	-70°C to +100°C	
	Temperature fluctuation	±0.3°C	
	Temperature variation in space	1.5°C	
	Temperature rate of change	Heat up rate: 5.0°C/min. Pull down rate: 2.0°C/min.	Heat up rate: 5.0°C/min. Pull down rate: 1.0°C/min.
	Temperature extremes achievement time	Heat up time: from +20°C to +100°C 30 min. Pull down time: from +20°C to -70°C 65 min.	
	Allowable heat load ^{*3}	700 W	2200 W
Allowable ambient conditions		0°C to +40°C/up to 75%rh	
Construction	Exterior material	Stainless steel plate: 18 Cr stainless steel plate, hairline finish	
	Test area material	Stainless steel plate: 18-8 Cr-Ni stainless steel plate, 2B polish	
	Heater	Nichrome strip wire heater	
	Cooler (dehumidifier)	Plate fin cooler, stainless steel tube cooler	
	Air circulator	Cross flow fan	Sirocco fan
	System	Mechanical cascade refrigerator system	
	Refrigerant	R-404A (R-449A is available on request), R-508A	
Capacity		306 L	800 L
Chamber total load resistance		100 kg	
Dimensions ^{*4}	Inside dimensions (W x H x D mm)	600 x 850 x 600	1000 x 1000 x 800
	Outside dimensions (W x H x D mm)	1010 x 1690 x 1273	1410 x 1853 (1983) x 1593
Weight		460 kg	695 kg
Augmented Reality Learn more  page 24		 ▲Exterior view	 ▲Exterior view
As representation, the products displayed in AR are temperature and humidity types.			

*1 The performance values are based on IEC60068-3-5:2001 under the conditions of a +23°C ambient temperature, relative humidity of 65±20%rh, rated voltage, and no specimen inside the test area.

*2 Lowest attainable temperature in an ambient temperature of 0°C to +30°C

*3 When temperature in chamber is +20°C


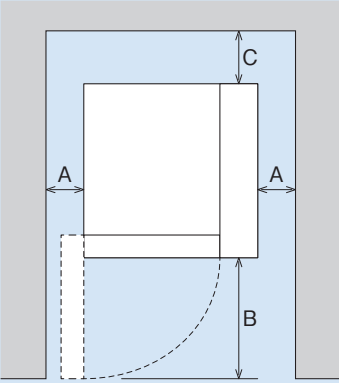
*4 Excluding protrusions. Dimension indicated in () includes protrusion.

Low GWP Refrigerant



R-449A is available on request.
(PR/PL/PSL/PU/PG only)

INSTALLATION REQUIREMENTS

Model	PR				PHP			PL				PSL		PDR		PDL		PCR	PU				PG	
	1	2	3	4	2	3	4	1	2	3	4	2	4	3	4	3	4	3	1	2	3	4	2	4
Maximum current (A)	200V AC 3ø 50/60 Hz																							
	18.5	20.0	22.0	34.0	17.0	17.8	26.4	22.5	23.0	36.0	32.0	48.5	34.0	44.5	35.5	47.0	23.5	14.5	15.0	28.0	24.5	45.0		
	220V AC 3ø 60 Hz *																							
	17.5	20.0	20.5	31.5	16.1	16.3	24.1	21.0	22.0	34.0	30.5	45.5	33.0	42.5	34.5	45.5	22.0	14.0	14.0	26.5	23.5	42.5		
	380V AC 3ø 50 Hz *																							
	8.5	10.0	19.5	8.6	15.4	10.0	11.0	22.0	18.0	30.0	17.5	27.0	18.5	29.0	11.0	9.0	10.5	13.5	17.5	23.0				
Humidifier water supply	Use pure water with a conductivity of 0.1 to 10 μ S/cm supplied from the tank.																		—					
	Drainage	Drain ports are positioned at the bottom of the rear panel (150 mm above the floor). Prepare 1 drain hose for temperature and humidity use and 1 drain hose for continuous water supply use (option). Hose outer diameter: 18 mm, inner diameter: 12 mm Length: approximately 1 m																						
Installation space																								
	Model	PR, PL, PU				PSL, PG		PHP			PDR, PDL		PCR											
		Type 1	Type 2	Type 3	Type 4	Type 2	Type 4	Type 2	Type 3	Type 4	Type 3	Type 4	Type 3											
	Side: A	Space to manipulate the cable port and adjuster feet, to connect the power supply and the water supply and drain pipes, and to perform maintenance is required. (We recommend 30 cm or more.)																						
	Front: B (cm)	70	80	120	80	120	70	80	120	80	120	80												
Rear: C	Space to pass the water drain hose through and to perform maintenance is required. (We recommend 60 cm or more.)																							
Top	60 cm or more																							

* Compliance with CE Marking

* The chamber does not come with a power cable.










Installation Simulation Tool (AR [Augmented Reality])

Read the QR code with a smartphone or tablet camera to start the web browser.*1

View the intended installation location (a floor) through the camera to check the installation image in the web browser.*2



Model / View with door open*3

<p>PR-1J PL-1J PU-1J*4</p> 	<p>PSL-4J PG-4J*4</p> 
 <p>PR-2J PL-2J PHP-2J PU-2J*4</p>	 <p>PDR-3J PDL-3J</p>
<p>PR-3J PL-3J PHP-3J PU-3J*4</p> 	<p>PDR-4J PDL-4J</p> 
 <p>PR-4J PL-4J PHP-4J PU-4J*4</p>	 <p>PCR-3J</p>
<p>PSL-2J PG-2J*4</p> 	

*1 This service is designed specifically for use on smartphones. It will also work on some tablets. Operation has been confirmed in the Safari and Google Chrome browsers. Use the camera function of your smartphone or tablet to read the 2D codes.

Recommended environment

- OS: iOS 14 or higher, Android 9.0 or higher
- Browser: Safari (latest version), Google Chrome (latest version)
- Even if you meet the above conditions, this service may not operate normally on your terminal.
- Not all Android terminals support AR. For details on terminals that support AR, access the following URL.
<https://developers.google.com/ar/devices?hl=en>



Check available devices

*2 Precautions

- These contents can be used free of charge, but you will be charged communication fees to access them.
- Possible causes for the contents not being displayed properly include the camera capturing a location with no flat surfaces, objects being present on the flat surfaces, and insufficient brightness in the location.
- This service may not operate properly due to the communication environment.
- Before using AR to capture images, thoroughly check the surrounding area to make sure it is safe.

*3 Initially, models are displayed with roughly their actual sizes. Stretch and pinch to change the dimensions of displayed models.

Use this service only as a reference. It does not provide any guarantees for actual installation of chambers.

*4 The products displayed in AR are temperature and humidity types, which are equipped with a temperature & humidity controller and water tank.

These types are displayed as a representative image. Actual temperature types (PU and PG) are equipped with a temperature controller but are not equipped with a water tank.

FITTINGS

- Drain hose (approx. 1 m) 1
- Condenser filter 1
- Cable port (I.D. \varnothing 50 mm on the left-side) 1
- Chamber lamp (bulb-type fluorescent light) 1
- Casters (free rolling type with leveling feet)..... 4
- Time signal terminal..... 2 contacts
- Specimen power supply control terminal..... 1
- Ethernet port (LAN port) 1
- USB memory port 1
- Viewing window 1
 - Type 1 to 3 W180 × H260 mm
 - Type 4 W295 × H380 mm
- Clean meter (PCR only)
- Duct meter (PCR only)

ACCESSORIES

- Glass fuse (7A)
 - Cable port rubber plug (\varnothing 50 mm) 1
 - Door key..... 2
 - Breaker handle stopper 1
 - Energy saving slit cover (PHP) 1
 - Fine wicks (except PU/PG) 1 (24 wicks)
 - Cloth wicks (PDR/PDL)..... 1 (20 wicks)
 - Connection duct (PDR/PDL)..... 2
 - Hose band (PDR/PDL)..... 1
 - Operation Manual (CD)..... 1 set
 - Warranty card 1
- * Shelves, shelf brackets, and power cables are not included.

Options

Utility

Power cable

- 2.5 m
- 5 m
- 10 m
- * If this option is not specified, the chamber does not come with a power cable.

Power plug

- 4P Plug
- * 200V AC only.

Power socket

- 100 V 3 A
 - 100 V 15 A (excluding Type1)
- Power outlets: 2
Location: Right-side
* 200V AC only.



Continuous water supply

A water circuit to supply pure water continuously to the chamber.

- Water supply coupling (with ion exchanger)
- Pure water coupling with pressure-reducing valve
- Pure water coupling without pressure-reducing valve



Pure water coupling (with pressure-reducing valve)

	Water Supply Coupling (With Ion Exchanger)	Pure Water Coupling	
		With Pressure-Reducing Valve	Without Pressure-Reducing Valve
Water pressure	0.05 MPa to 0.50 MPa (Gauge)	0.05 MPa (Gauge)	0.03 MPa (Gauge)
Flow rate	1.3 L/minute or more		
Conductivity	—	0.1 μS/cm to 10 μS/cm	
Location	Lower left rear side		Upper left rear side
Connectable items	Only a steel pipe (or a PVC pipe) can be connected.		Only a hose can be connected.

* Connection of the chamber to the water supply equipment shall be performed by the user.

* The ion exchanger must be replaced periodically.

*To prevent damage in the event of water leakage when installing the following optional products, a dew tray (page 36) and other preventive measures can be prepared.

- Continuous water supply
- Water purifier
- Water-cooled refrigeration

Water purifier (reverse osmosis)

Use to continuously supply pure water.

- WS-1
 - Power: AC100V 50/60Hz 0.4A
 - AC200V 50/60Hz 0.2A
 - AC220V 50/60Hz 0.2A
 - AC230V 50/60Hz 0.2A



- Produced water capacity: 12 L/h (Water temperature: 25°C)
- Size: W480 × H480 × D280 mm
- Produced water (pure water) supply: One or two couplings
- Location: Chamber ceiling

Water-cooled refrigeration

To reduce the effect of exhaust heat, this option changes the refrigeration system to a water-cooled condenser.

- Fittings: Compressor cooling fan
Water supply and drain ports
Water suspension relay

Additional water supply tank

The additional water supply tank complements the water volume of the standard-equipped tank, to allow continuous operations for long periods.

Effective water volume:

Approximately 13L

- * When the tank is attached, the chamber height increases by 215mm



Water tank

For supplying water to the chamber's fixed tank.

- Water tank with cart
 - Size: W600 × H920 × D348 mm
 - Tank (10 L, with cock) × 3
- Water tanks 10 L × 1



Tank with cock (cart included)



Tank with nozzle

Options

Observation

Wide-view door

Almost the entire surface of the door is made of glass for test area inspection, even when testing is on process.

- Upper limit temperature +100°C
- Upper limit temperature +120°C

Effective view:

- Type 2 W470 × H720 mm
- Type 3 W570 × H820 mm
- Type 4 W970 × H970 mm

* Refer to specification sheet for temperature rate of change, extremes achievement time and allowable heat load.

* The door cannot be locked.



Wide-view door with hand-in ports

This option features hand-in ports on a standard door, to manipulate the specimen even during testing.

Hand-in ports' inner diameter: 130mm

Number of hand-inports: One or two pairs

Accessory: Rubber gloves

* Refer to specification sheet for temperature rate of change, extremes achievement time and allowable heat load.




Roller blind for wide-view window

Spring screen that can be attached to obscure the view of the inside of the chamber from the viewing window. Shade grade 1 (black)



Electrochromic viewing window

Switching opacity to transparent state by chamber lamp. The test area can be observed while the chamber lamp is on.

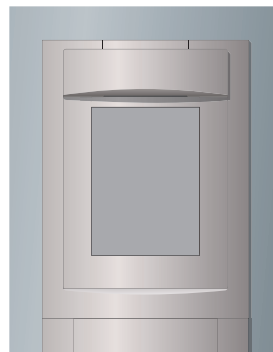

Lamp off



Lamp on



Options

Observation

Door with hand-in ports

This option features hand-in ports on a standard door, to manipulate the specimen even during testing.

Number of hand-in ports:

Type 2: One pair

Type 3: One pair

Type 4: One pair or two pairs

Hand-in ports' inner diameter:

130 mm

Accessory: Rubber gloves



Door without viewing window

Plain door ideal to test specimens affected by light.

* There is no lamp installed in the test area with this option.



Inner glass door


A glass door is provided between the test area and the chamber door to observe specimens. Select hand-in ports and chamber door viewing window.

Hand-in port: ID 130mm with radial rubber seal & rubber gloves


Model	Inner Door	Wipers	Hand-in Ports
Types 1 to 3	Single door	1	1 pair
Type 4	Hinged double doors	2	2 pairs
			4 pairs
			6 pairs




Inner glass door with a wiper (Type 1)

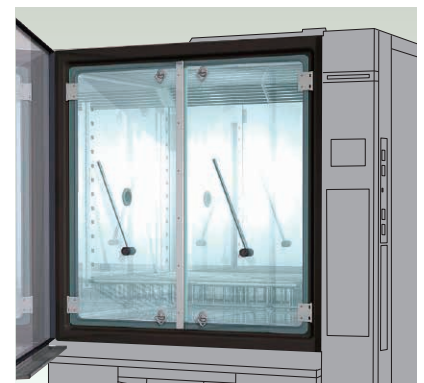

Inner glass door with wipers (Type 4)

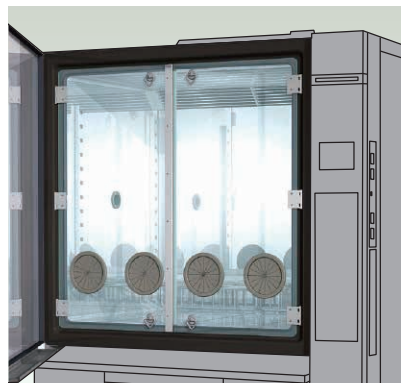

Inner glass door with two pairs of hand-in ports

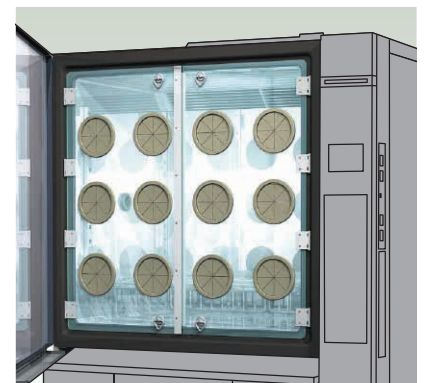

Inner glass door with six pairs of hand-in ports

- * Inner glass door cannot be installed on the PCR model.
- * Wiper's installation differs depending on the configurations.
- * Wipers are not provided to chambers controlling only temperature.
- * The lock release mechanism equipped as standard on the Type 4 is removed.
- * Refer to specification sheet for temperature rate of change, extremes achievement time and temperature variation in space.

Options

Specimen setting



Shelf/shelf bracket

Used to place the specimen inside the chamber.

< Shelf >

- 18-8Cr-Ni
Stainless steel

- Resin-coated
 - * Upper limit temperature: +100°C
 - * PU and PG only



Dimensions & weight:

- For Type 1: 350 × 467 mm, 1.0kg
- For Type 2: 550 × 467 mm, 1.5kg
- For Type 3: 750 × 567 mm, 2.2kg
- For Type 4: 750 × 967 mm, 6.6kg
- For PSL/PG-2: 550 × 567 mm, 1.6kg

Load capacity for the standard shelf
 Type 1 to 3: 10 kg
 Type 4: 30 kg

< Shelf bracket >

- 18-8Cr-Ni Stainless steel
1 set (2 pieces)



Heavy-duty shelf

Used to hold heavy specimens.

* To install heavy-duty shelves from 50 kg, reinforcement of the chamber structure is necessary.

Load capacity (per shelf):

- 30kg (Except PDL/ PDR/ PCR)
- 50kg (Except PDL/ PDR/ PCR)
- 80kg (Only for type 4, 150°C spec., except PHP/PDR/PDL)
- 100kg (A set of 5 shelves, only for type 4, except PDR/ PDL)

Load Capacity per Shelf	Capacity of Shelf Support Pole	Floor Load Capacity	Chamber's Total Load Capacity	Shelf Weight (Per Shelf)	Max. Qty. in Chamber
30 kg	90 kg	70 kg	100 kg	Type 1: 1.8 kg Type 2: 2.9 kg Type 3: 4.3 kg PSL/PG2: 3.4 kg	3
50 kg	100 kg	70 kg	100 kg	Type 1: 2.3 kg Type 2: 3.4 kg Type 3: 5.1 kg Type 4: 12.1 kg PSL/PG2: 4.0 kg	2
80 kg	100 kg	70 kg	100 kg	9.3 kg	2
100 kg	A special rack is installed in the test area to accommodate 5 shelves.(Rack weight:56kg)		500 kg	13 kg	5


* Weight of shelf (ves) + Specimen on shelf (ves) efloor + special rack.

Specimen basket

For small specimens that cannot be placed directly on the shelf.

Material: Stainless steel (4 mesh)

- Large
 - Dimensions: W700 × H35 × D450 mm
 - Load capacity: 5 kg (equally distributed load)
 - Qty. per shelf: Type 3: 1
Type 4: 2
- Small
 - Dimensions: W350 × H35 × D270 mm
 - Load capacity: 3 kg (equally distributed load)
 - Qty. per shelf: Type 1: 1
Type 2: 2
Type 3: 4
Type 4: 6

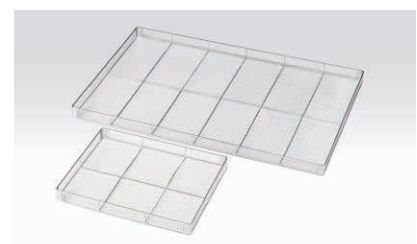

- * Place the specimen baskets on the shelf.
- * Do not use when exceeding the shelf load capacity.
- * Tests may not satisfy standard performance if the air flow is blocked, so ensure sufficient space around the specimen baskets.

Options

Specimen setting

Floor reinforcement

Enhances the floor load capacity inside the chamber.

- Up to 100 kg
- Up to 200 kg
- Up to 300 kg
- * Standard specification: up to 70 kg

Precision inner chamber

An aluminum box inside the chamber allows to reduce the air velocity and maintain the required temperature and humidity distribution.

Velocity: to 0.5 m/sec.


Temperature & humidity fluctuation:
± 0.5°C/± 2.5%/rh

Effective cross section & load capacity :

- Type 1 W335 × H285 mm, up to 20kg
- Type 2 W335 × H435 mm, up to 20kg
- Type 3 W435 × H585 mm, up to 30kg
- Type 4 W835 × H685 mm, up to 30kg

Accessories: Shelves and shelf brackets
(2 sets)

* Refer to specification sheet for temperature rate of change, extremes achievement time and allowable heat load.

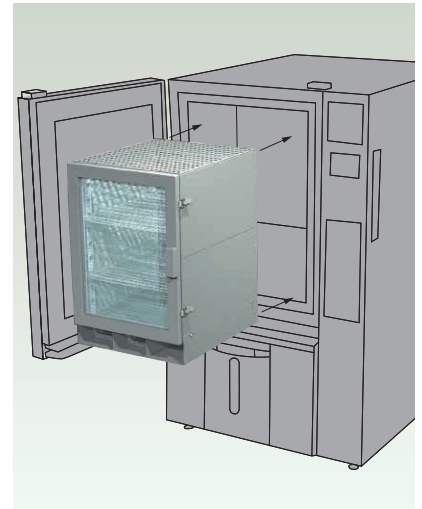

Additional cable port

Provided in addition/ replacement of the standard cable port (left side). Comes with a cap and a rubber plug.

- ø25 mm
- ø50 mm
- ø70 mm
- ø100 mm
- ø150 mm
- Flat cable port

* When installed on the right side, an external drip pan is also included.



Left-side (chamber interior)



Right-side

Port type		Model				PR			PHP			PL				PSL		PDR		PDL		PCR				PU				PG	
		1	2	3	4	2	3	4	1	2	3	4	2	4	3	4	3	4	3	4	1	2	3	4	2	4					
Right	φ 50mm	—	●	●	●	●	●	●	—	●	●	●	●	●	●	●	●	●	—	—	●	●	●	●	●	●					
	φ 50mm around wiring board inside the wall	—	●	●	●	●	●	●	—	●	●	●	●	●	●	●	●	●	—	—	●	●	●	●	●	●					
	φ 100mm	—	●	●	●	●	●	●	—	●	●	●	●	●	●	●	●	●	—	—	●	●	●	●	●	●					
	φ 100mm around wiring board inside the wall	—	—	●	●	—	●	●	—	—	●	●	—	●	●	●	●	●	—	—	—	●	●	—	●	●					
Left	φ 25mm	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○					
	φ 50mm	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○					
	φ 70mm	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●					
	φ 100mm	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○					
	φ 150mm	—	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	—	●	●	●	●	●					
	Flat cable port	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●	●					
Ceiling	φ 25mm	○	○	○	○	—	—	—	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○					
	φ 50mm	○	○	○	○	—	—	—	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○					
	φ 70mm	●	●	●	●	—	—	—	●	●	●	●	●	●	●	●	●	●	●	●	—	●	●	●	●	●					
	φ 100mm	○	○	○	○	—	—	—	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○	○					
	φ 150mm	—	—	●	●	—	—	—	—	—	●	●	●	●	●	●	●	●	●	●	—	—	—	●	●	●					
	Flat cable port	●	●	●	●	—	—	—	●	●	●	●	●	●	●	●	●	●	●	●	—	●	●	●	●	●					

● Retrofit is not available. ○ Retrofit is available.

Options

Specimen setting

Cable port rubber plug

Comes with the cable port.

- $\phi 25$ mm
- $\phi 50$ mm
- $\phi 100$ mm
- Spiral-wrapped plug ($5 \times 50 \times 2000$ mm)
- For the flat cable port



$\phi 50$ mm

Spiral-wrapped type
* Cut the silicone sponge so that the roll fits in the port.

For flat cable port

Cable port dew tray (for left side)

Catches dew that comes out of the cable port.

Location: Left-side

Model	Size (W × Dmm)
Type 1	300×50
Type 2	510×50
Type 3-4	700×50
PDR/PDL	600×50



EZ connect cable port plug for power supply

Wires that go through this cable port plug have a terminal at both ends.

This option ease the power cable connection between specimen and external device.

Spec.: AC 6V to 24V 0.1 to 3A

DC 1.5V to 60V 0.1 to 3A


Interior terminals: Terminals on insulated jig plate, 10P

Exterior terminals: Block terminals with magnet, 10P

Temperature/ humidity range:

-70°C to $+180^{\circ}\text{C}$ / 20%rh to 98%rh

* Based on cable port $\phi 25\text{mm}$ and $\phi 50\text{mm}$.

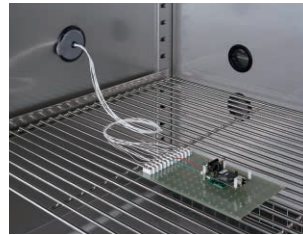

Interior terminal



Exterior terminal



EZ connect cable port plug for measurement

This port plug equips with a terminal box on interior wall, which facilitates the wiring work inside the test area.


Spec.: DC no more than 500V, 5A

Terminals: 20ch

More than $1\Omega \times 10^{12}\Omega$ as insulation resistance

Temperature/ humidity range:

-70°C to $+150^{\circ}\text{C}$ / 20%rh to 98%rh

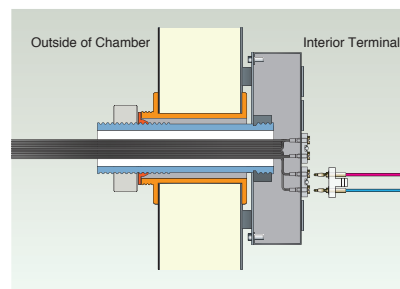

Options

Performance

DC inverter refrigeration

Able to reduce power consumption when operating at low temperatures of 0°C or below as well as shorten temperature pull-down time.

- 100°C Specification
- 150°C Specification
- * 200V AC only


Upper limit modification

Enables tests over 100°C.

- Upper limit temperature +150°C
- Upper limit temperature +180°C (except PSL-4, PG-4)
- * Refer to specification sheet for temperature rate of change, and temperature variation in space.

Defrost circuit

Defrosts the refrigeration circuit.

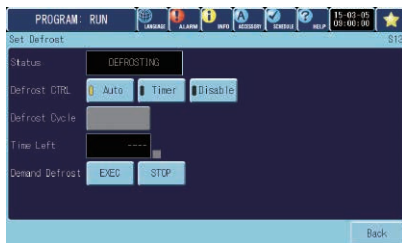


Frost relief valve

To reduce frosting on the evaporator during continuous operation at room temperature (25°C) or at a low temperature.

Airflow adjuster


Used when tests require low airflow velocity or a certain velocity of airflow.

Setting value range: 4 levels



Lower temperature & humidity range

Testing can be performed at low temperature and humidity (+5°C / 5%rh) where static electricity tends to be generated.

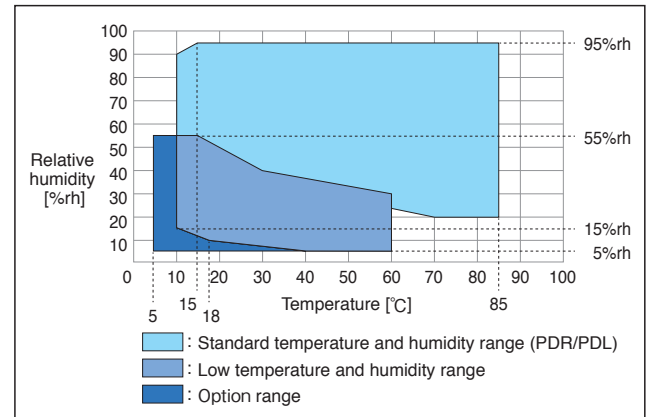


Frost-free circuit

Prevents frost from accumulating on the refrigeration circuit to allow long-term continuous operation.

Operating ambient temp. range:

Approx. +10°C to +40°C

* Except the PR-1/PL-1/PU-1/PHP

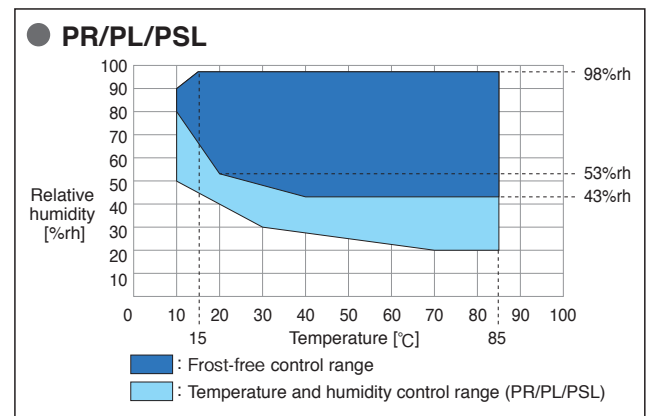

Options

Performance

Specimen temperature control

Sensors are attached to the specimen to allow exposure tests that provide accurate temperature stress to the specimen.

- Insulated type
- Non-insulated type



Capacitive humidity sensor

Attached in place of the wet bulb wick.

Measurement range: 0%rh to 100%rh

Accuracy: $\pm 2\%$ rh

(-20°C to $+40^{\circ}\text{C}$ and 0%rh to 90%rh)



Time up output

This option enables turning the power to the specimen ON or OFF with contact signal output when the time is up by using the timer function on the temperature (humidity) controller.



Time signal terminal

Adds additional terminals to the standard time signal terminals.



Temp. & humid. SP attainment output

When the temperature (humidity) in the chamber reaches the set values, the chamber sends out a contact signal.

It synchronizes the power supply to the specimen, the timing for measurements or to prevent dew from condensing on the specimens.

Applying DC power supply

Capable of applying voltage to the specimen, used for bias testing. The DC power supply unit synchronizes with constant and program operations, and can be set for each temperature and humidity program step.

Rated voltage	5V	12V	15V	24V	48V
Rated current	60A	27A	22A	14A	7A
Voltage setting range	1.0 to 5.5V	2.4 to 13.2V	3.0 to 16.5V	4.8 to 26.4V	9.6 to 52.8V



Options

Measurement

I/O Interface

Communication ports to connect the chamber to a PC and a device and using communication commands.

- RS-485* (D-sub 9-pin × 2)
- RS-232C (D-sub 9-pin × 1)
- GPIB* (IEEE488)

* Up to 16 chambers can be connected to a single PC.

Communication cables

- RS-485 5 m / 10 m / 30 m
- GPIB 2 m / 4 m

Temperature (humidity) recorder wiring

Preparation of a power cable, temperature sensor, relative humidity signal and a grounding wire for additional installation in the future.

Paperless recorder

A temperature & humidity recorder that utilizes a liquid-crystal display fitted with a touch-panel.

Display: 5.7inch color touch panel

Scan interval: 5 sec. (default)

Internal recording media:Flash memory 8MB

External recording media:CF memory card(Supplies with a 256 MB CF card)USB flash drive

< Temperature type >

No. of input channel:Temperature 1
(5 more channels can be turned ON)

< Temperature & humidity type >

No. of input channel:Temperature 1,
Humidity 1

(4 more channels can be turned ON)



Temperature (humidity) recorder

Records the temperature and humidity of each section such as the temperature inside the chamber.

Recording method: Dot

Recording paper: Effective width 100 mm

No. of inputs:

< Temperature & humidity type >

Temperature 5, Humidity 1

–50°C to +100°C/0%rh to 100%rh

–50°C to +150°C/0%rh to 100%rh

–100°C to +100°C/0%rh to 100%rh

–100°C to +150°C/0%rh to 100%rh

–100°C to +200°C/0%rh to 100%rh

< Temperature type >

Temperature 6

–50°C to +100°C

–100°C to +100°C

–100°C to +200°C



Thermocouple

Attached to specimen to measure specimen temperature.

Thermocouple with a brass ball tip
Thermocouple type T
(Copper/Copper-Nickel)

- 2 m
- 4 m
- 6 m



Recorder output terminal

- Temperature, humidity, and heater output

This terminal outputs the temperature and relative humidity in the test area.



- Dry/wet bulb temperature



Terminal board for dry-bulb/wet-bulb sensors in the chamber.



Wet bulb wick

This option contains replacement wicks.

- Fine wicks (non-woven fabric)
FW-5 (for the PR, PL, PSL, and PHP): 24 wicks
FW-6 (for the PDR, PDL, and PCR): 24 wicks



FW-5

FW-6

- Cloth wicks (gauze)
For the PDR and PDL: 20 wicks



Power meter

This option displays the integral power consumption of the chamber.

Display range: 0 to 9999.99 kWh

External memory: SD memory card

Location: Instrumentation panel

* The SD memory card is not included.



Folding table

A folding table is equipped on the right side of the chamber.

The table can be used when a measuring instrument, PC, or other device is connected.

Table dimensions: W410 × D300 mm

Load capacity: 20 kg



Options

Safety

Overcool protector

If the temperature inside the chamber decreases excessively, the chamber stops operating to prevent the specimens from being damaged.

Additional overheat protector

Additional preventive measures can be taken for excessive temperature rise in the chamber, in addition to the standard equipped overheat protector.



Alarm output terminal

If the safety device of the chamber is activated, external alarm terminal will notify it to a remote point.

Operation:

When connecting with N.O. contact (normally open contact), output “close” contact.

When connecting with N.C. contact (normally close contact), output “open” contact.

Current-carrying capacity: 250 V AC, 3 A

Accessory: Plug

Location: Right side or within the control board (retrofit is not available)

* Please connect the alarm circuit by customer.

* This option can also be installed inside the electrical compartment.

Please inquire for the details.

External device alarm input terminal

Equips the chamber with a terminal that is used to stop the operation of the chamber in the event that an external device to which the chamber is linked malfunctions.

Door opening signal output terminal

Equips the chamber with a terminal that outputs the door open status.

Capable of controlling an external device that operates along with door operation and records the temperature disturbance history.

Status indicator light

Select light color, lighting, and blinking or buzzer sound.

- 1 level, light: 1 color, height: 534 mm
 - 2 levels, light: 2 colors, height: 574 mm
 - 3 levels, light: 3 colors, height: 614 mm
 - 4 levels, light: 4 colors, height: 654 mm
- Pole length: 290 mm

* The pole can be shortened in units of 10 mm to a minimum height of 50 mm.



Rotating signal light

The rotating signal lights up when an error occurs.

Color of the signal:

- Red
- Yellow



Trouble buzzer

Buzzer notification when an error occurs.

Emergency stop pushbutton

Stops the chamber immediately.



Power key switch

Used to manage/restrict the chamber usage.



Power indicator

The operator can verify if the breaker is ON or OFF from the chamber front.



Main power switch

The main power switch allows turning the power ON and OFF from the chamber front.

* 380 V AC and 400 V AC only.



Options

Safety

Pressure relief vent

To reduce an explosive force by releasing pressure when the chamber pressure suddenly goes up.

Pressure relief vent: W300 × D300 mm
Outside dimension: 200 mm higher than the standard height.

* The pressure relief port is not intended to guarantee safety against explosion.



Dew drip prevention

To prevent dew that has formed on the chamber ceiling from dripping onto specimens.

* The height is 20 mm smaller than the standard inside dimensions.
* Refer to specification sheet for temperature rate of change, extremes achievement time.



Safety door lock

• Dial combination safety door lock
The dial mechanism gives more secure door locking.

Dial combination



• Lever handle safety door lock
The rotation mechanism with levers gives more secure door locking.
* In case of Type 4, unlocking device is not equipped.

Lever handle



Operation panel cover

A cover for the operation panel. (Plastic)



Anchoring fixtures

Used to fix the chamber to the floor.

* Anchoring fixtures when installing the dew tray are also available.



Evaporator frost check window

This window is installed in the test area and is used to check whether frost has accumulated on the cooler.

Diameter: 55 mm



Chamber dew tray

A chamber dew tray is installed below the chamber in the unlikely case there would be water leakage.



Test area low-silicone

Reduces the production of silicone gas (siloxane) in the test area.

Brake oil protection

Changes resin parts (water tank front cover, door dew tray, chamber dew tray) to stainless steel.

Finned sheathed heater

Changes the heater to a sheathed heater with fins to lower the surface temperature of the heater, decrease corrosion, and reduce defective insulation.

Stainless steel evaporator

Changes the plate fin cooler (also used as a dehumidifier) to stainless steel, which improves the corrosion resistance.

* Refer to specification sheet for temperature rate of change, extremes achievement time and allowable heat load.

Air circulator removed for move-in

To prevent damage caused by height restrictions, the air circulator for type 4 chambers is not mounted on the chamber during shipment.

* The air circulator must be installed separately.

Type	W×H×Dmm
1	1010×30×1030
2	1010×30×1230
3 (PSL/PG-2)	1110×30×1430
4	1510×30×1430
PSL/PG-4	1510×30×1750
Dehumidifier unit for PDL/PDR	875×30×1430

* The chamber dew tray is a product for on-site installation.
The price does not include the installation cost. Contact your distributor or ESPEC for details.

Options


Documents

Operation manual


- CD
- Booklet

Reports & certificates


- Testing and inspection report
- Test data
- Temperature (& humidity) uniformity measurement
- Calibration report
- Calibration certificate
- Traceability certificate
- Traceability system chart

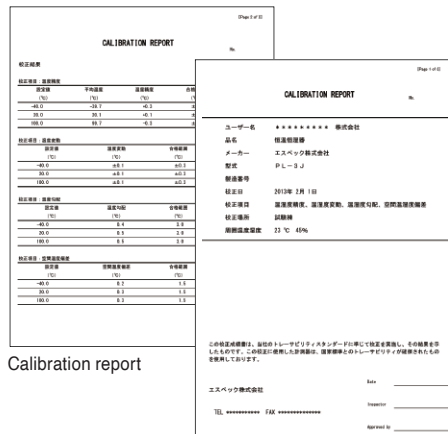

Calibration report

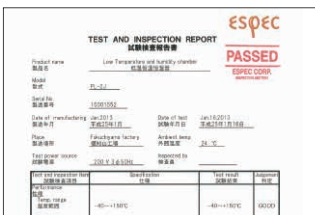


Testing and inspection report

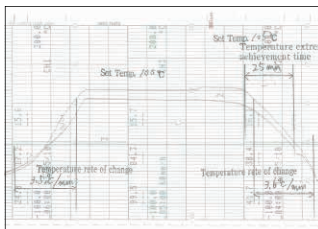

Standard test data




Calibration certificate



Traceability certificate

Temperature and humidity uniformity measurement data

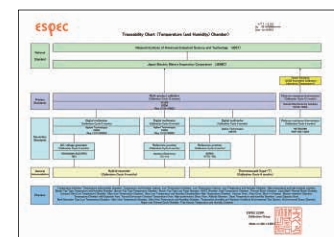

Traceability system chart

Safety precautions

- Do not use specimens which are explosive or inflammable, or which contain such substances. To do so could be hazardous, as this may lead to fire or explosion.
- Do not place corrosive substances in the chamber. If corrosive substances are generated by the specimen, the life of the chamber may be significantly shortened specifically because of the corrosion of stainless steel and copper and because of the deterioration of resin and silicon. An optional stainless steel evaporator, which is designed to improve the corrosion resistance of the chamber, is available.
- Do not place life forms or substances that exceed allowable heat generation.
- Be sure to read the operation manual before operation.

Platinous J Series Options

Utility, Observation, Specimen setting

● Retrofit is not available. ○ Retrofit is available.

Page	OPTION	PR	PHP	PL	PSL	PDR/PDL	PCR	PU	PG
P.26	Power cable	●	●	●	●	●	●	●	●
	Power plug *1	●	●	●	●	●	●	●	●
	Power socket *1	●	●	●	●	●	●	●	●
	Continuous water supply	○	○	○	○	○	○	—	—
	Water purifier	○	○	○	○	○	○	—	—
	Water-cooled refrigeration	●*2*7	—	●*2*7	●*7	—	●	●*2*7	●*7
	Additional water supply tank	○	○	○	○	○	○	—	—
	Water tank	○	○	○	○	○	○	—	—
P.27	Wide-view door *3*7	○	—	○	—	—	—	○	—
	Wide-view door with Hand-in ports *2*7	●	—	●	—	—	—	●	—
	Roller blind for wide-view window *3*7	●	—	●	—	—	—	●	—
	Electrochromic viewing window	●	●	●	●	●	●	●	●
P.28	Door with hand-in ports *3	●	●	●	●	●	—	●	●
	Door without viewing window	●	●	●	●	●	●	●	●
	Inner glass door	●	●	●	●	●	—	●	●
P.29	Shelf/shelf bracket (Stainless steel)	○	○	○	○	○	○	○	○
	Shelf (Resin-coated)	—	—	—	—	—	—	○	○
	Heavy-duty shelf (30 kg) *4	○	○	○	○	—	—	○	○
	Heavy-duty shelf (50 kg) *5	○	○	○	○	—	—	○	○
	Heavy-duty shelf (80 kg) *6	●	—	●	●	—	—	●	●
	Heavy-duty shelf (100 kg) *6	●	●	●	●	—	—	●	●
	Specimen basket	○	○	○	○	○	○	○	○
P.30	Floor reinforcement (100 kg)	○	○	○	○	—	—	○	○
	Floor reinforcement (200 kg/300 kg)	●	●	●	●	—	—	●	●
	Precision inner chamber	○	○	○	○	—	—	○	○
	Additional cable port	Inquire for details.							
P.31	Cable port rubber plug	○	○	○	○	○	○	○	○
	Cable port dew tray (for left side)	●	●	●	●	●	●	●	●
	EZ connect cable port plug for power supply	○	○	○	○	○	○	○	○
	EZ connect cable port plug for measurement	○	○	○	○	○	○	○	○

*1 Applicable only to 200V AC.

*2 Type 3 and 4 only.

*3 Excluding Type 1.

*4 Excluding Type 4.

*5 If the chamber has been reinforced, equipment can be added.

*6 Type 4 only.

*7 Contact us for availability of this option with low GWP refrigerant type product.

Platinous J Series Options

Performance, Measurement

● Retrofit is not available. ○ Retrofit is available.

Page	OPTION	PR	PHP	PL	PSL	PDR/PDL	PCR	PU	PG
P.32	DC inverter refrigeration *1 *2 *3	—	—	●	—	—	—	●	—
	Upper limit modification (+150°C)	●	—	●	●	—	—	●	●
	Upper limit modification (+180°C)	●	—	●	●*4	—	—	●	●*4
	Defrost circuit	●*1	—	●*1	●	●	●	●*1	●
	Frost relief valve	●	—	●	●	●	●	●	●
	Airflow adjuster	○	—	○	○	—	—	○	○
	Lower temperature & humidity range	—	—	—	—	●	—	—	—
	Frost-free circuit	●*1	—	●*1	●	●	●	●*1	●
P.33	Specimen temperature control	○	○	○	○	○	○	○	○
	Capacitive humidity sensor	●	●	●	●	●	●	—	—
	Time up output	●	●	●	●	●	●	●	●
	Time signal terminal	●	●	●	●	●	●	●	●
	Temp. & humid. SP attainment output	●	●	●	●	●	●	●	●
	Applying DC power supply	○	○	○	○	○	○	○	○
P.34	Interface	○	○	○	○	○	○	○	○
	Communication cables	○	○	○	○	○	○	○	○
	Temperature (humidity) recorder wiring	○	○	○	○	○	○	○	○
	Paperless recorder	○	○	○	○	○	○	○	○
	Temperature (humidity) recorder	○	○	○	○	○	○	○	○
	Thermocouple	○	○	○	○	○	○	○	○
	Recorder output terminal (temperature, humidity, and heater output)	○	○	○	○	○	○	—	—
	Recorder output terminal (dry [wet] bulb temperature)	○	○	○	○	○	○	○	○
	Wet bulb wick	○	○	○	○	○	○	—	—
	Power meter	○	○	○	○	○	○	○	○
Folding table *5	●	●	●	●	●	—	●	●	

*1 Excluding Type 1.

*2 Applicable only to 200V AC.

*3 Contact us for availability of this option with low GWP refrigerant type product.

*4 Type 4 only.

*5 Type 3 and 4 only.

Platinous J Series Options

Safety, Documents

● Retrofit is not available. ○ Retrofit is available.

Page	OPTION	PR	PHP	PL	PSL	PDR/PDL	PCR	PU	PG
P.35	Overcool protector	○	○	○	○	○	○	○	○
	Additional overheat protector	○	○	○	○	○	○	○	○
	Alarm output terminal	○	○	○	○	○	○	○	○
	External device alarm input terminal	●	●	●	●	●	●	●	●
	Door opening signal output terminal	○	○	○	○	○	○	○	○
	Status indicator light	○	○	○	○	○	○	○	○
	Rotating signal light	○	○	○	○	○	○	○	○
	Trouble buzzer	○	○	○	○	○	○	○	○
	Emergency stop pushbutton	○	○	○	○	○	○	○	○
	Power key switch	○	○	○	○	○	○	○	○
	Power indicator	○	○	○	○	○	○	○	○
	Main power switch *1	○	○	○	○	○	○	○	○
	P.36	Pressure relief vent *2	●	—	●	●	●	—	●
Safety door lock		●	●	●	●	●	●	●	●
Anchoring fixtures		●	●	●	●	●	●	●	●
Chamber dew tray		●	●	●	●	●	●	●	●
Dew drip prevention		●	Standard equipment	●	●	●	—	●	●
Operation panel cover		●	●	●	●	●	●	●	●
Evaporator frost check window		●	—	●	●	—	—	●	●
Test area low-silicone		●	●	●	●	—	—	●	●
Brake oil protection *3		●	—	●	—	—	—	●	—
Finned sheathed heater *4		●	—	●	●	—	—	●	●
Stainless steel evaporator *5		●	—	●	—	—	—	●	—
Air circulator removed for move-in *6	●	●	●	●	●	—	●	●	
P.37	Operation manual	○	○	○	○	○	○	○	○
	Reports & certificates	●	●	●	●	●	●	●	●

*1 Applicable only to 380 V/400 V AC.

*2 Excluding Type 1.

*3 Type 3 and 4 only.

*4 Applicable only to 200V AC.

*5 Contact us for availability of this option with low GWP refrigerant type product.


*6 Type 4 only.

Larger model (816L & 1000L)


The test samples are getting larger and heavier due to the changes in market needs. The demand for assembly, module or completed product testing is increasing because individual parts testing can be checked stand alone performance only but assembly testing can be evaluated the test samples in a correct, stable and proper manner which is defined in the functional requirements provided by the customer. Therefore, the larger test area sizes are added to the lineup to meet the latest trends in testing.

on request

Capacity	816 L	1000 L
Temperature & humidity range	-40°C to +100°C (+150°C/+180°C with high-temperature control range expansion option installed)/20%rh to 98%rh	
Temperature rate of change	Heat up rate: 2.5°C/min; Pull down rate: 1.5°C/min	
Temperature extremes achievement time	Heat up: +20°C to +100°C: 35 minutes Pull down: +20°C to -40°C: 50 minutes	Heat up: +20°C to +100°C: 40 minutes Pull down: +20°C to -40°C: 55 minutes
Inside dimensions (W x H x D mm)	1200 x 850 x 800	1000 x 1000 x 1000
Outside dimensions (W x H x D mm)	1610 x 1690 (including protrusions: 1815) x 1273	1410 x 1840 (including protrusions: 1965) x 1473

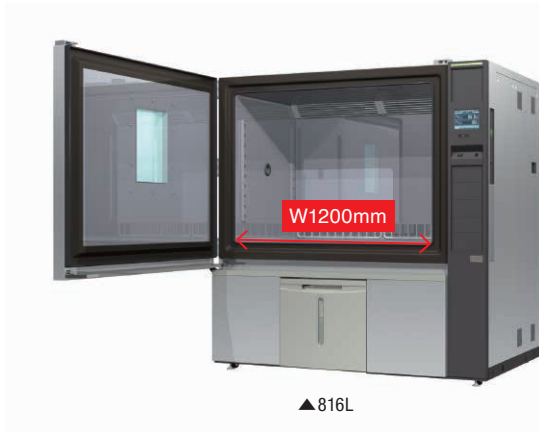

● Temperature & Humidity Control Range

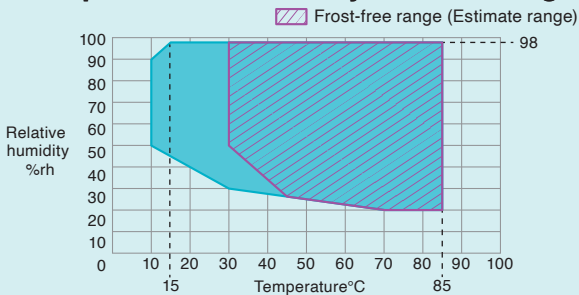

* With no specimen and under ambient temperature at +23°C.
 * Restrictions on continuous humidity operation at +40°C or lower because of frost on the cooler.

For IoT/5G

Systems for OTA Tests/Wireless Tests in Temperature Environments

RF Anechoic Box-Type Low Temperature Chamber

- An RF anechoic chamber and a temperature chamber combined, allowing you to execute performance tests for small communication modules under extreme temperature conditions.
- Ideal for wireless protocol tests that require shorter distance between antenna and DUT than wireless RF performance tests.
- Ensures an attenuation rate of 60dB or greater in 4.0 to 6.0GHz frequency bands.
- The interior of the RF anechoic box can be precisely controlled from low temperature to high temperature.



▲PUAN-4

Model	PUAN-3	PUAN-4
Frequency range / Attenuation rate	0.7GHz to 2.4GHz/45dB~ 2.4GHz to 4GHz/50dB~ 4GHz to 6GHz/60dB~	
Temperature range	-40 °C to +100 °C	
Inside dimensions (W x H x D mm)	300 x 550 x 500	750 x 750 x 550
Watch the video for more information		

Discover test solutions for IoT/5G/Optical communication devices

Introduction of environmental test chambers and measurement systems for IoT/5G/optical communication

ESPEC provides environmental test chambers and measurement systems all over the world, for much efficiency of evaluation of test standards, reliability, temperature characteristics and antenna performance.



<https://www.espec.co.jp/english/products/search/market/iot-5g-optical/>

ESPEC CORP. <https://www.espec.co.jp/english>

Head Office

3-5-6, Tenjinbashi, Kita-ku, Osaka 530-8550, Japan
Tel: 81-6-6358-4741 Fax: 81-6-6358-5500

ESPEC NORTH AMERICA, INC.

Tel: 1-616-896-6100 Fax: 1-616-896-6150

ESPEC EUROPE GmbH

Tel: 49-211-361850-0

ESPEC ENVIRONMENTAL CHAMBERS

SALES AND ENGINEERING LTD. STI. (Turkey)

Tel: 90-212-438-1841 Fax: 90-212-438-1871

ESPEC ENVIRONMENTAL EQUIPMENT (SHANGHAI) CO., LTD.

Head Office

Tel: 86-21-51036677 Fax: 86-21-63372237

BEIJING Branch

Tel: 86-10-64627025 Fax: 86-10-64627036

GUANGZHOU Branch

Tel: 86-20-83317826 Fax: 86-20-83317825

SHENZHEN Branch

Tel: 86-755-83674422 Fax: 86-755-83674228

SUZHOU Branch

Tel: 86-512-68028890 Fax: 86-512-68028860

TIANJIN Branch

Tel: 86-22-26210366 Fax: 86-22-26282186

XI'AN Branch

Tel: 86-29-88312908 Fax: 86-29-88455957

CHENGDU Branch

Tel: 86-28-88457756 Fax: 86-28-88474456

WUXI Branch

Tel: 86-510-82735036 Fax: 86-510-82735039

ESPEC TEST TECHNOLOGY (SHANGHAI) CO., LTD.

Tel: 86-21-68798008 Fax: 86-21-68798088

ESPEC ENGINEERING (THAILAND) CO., LTD.

Tel: 66-3-810-9353 Fax: 66-3-810-9356

ESPEC ENGINEERING VIETNAM CO., LTD.

Tel: 84-24-22208811 Fax: 84-24-22208822

ISO 9001 (JIS Q 9001)

Quality Management System Assessed and Registered

ESPEC CORP. has been assessed by and registered in the Quality Management System based on the International Standard ISO 9001:2015 (JIS Q 9001:2015) through the JSA Solutions Co.,Ltd.

* The organization of these certificates is
ESPEC CORP. Japan.



ISO 27001 (JIS Q 27001)

Quality Management System Assessed and Registered

* The organization of these certificates is
ESPEC CORP. Japan.



ISO 14001 (JIS Q 14001)

Environmental Management System Assessed and Registered

* The organization of these certificates is
ESPEC Group Japan.



● Specifications are subject to change without notice due to design improvements.

● Corporate names and trade names mentioned in this catalog are trademarks or registered trademarks.